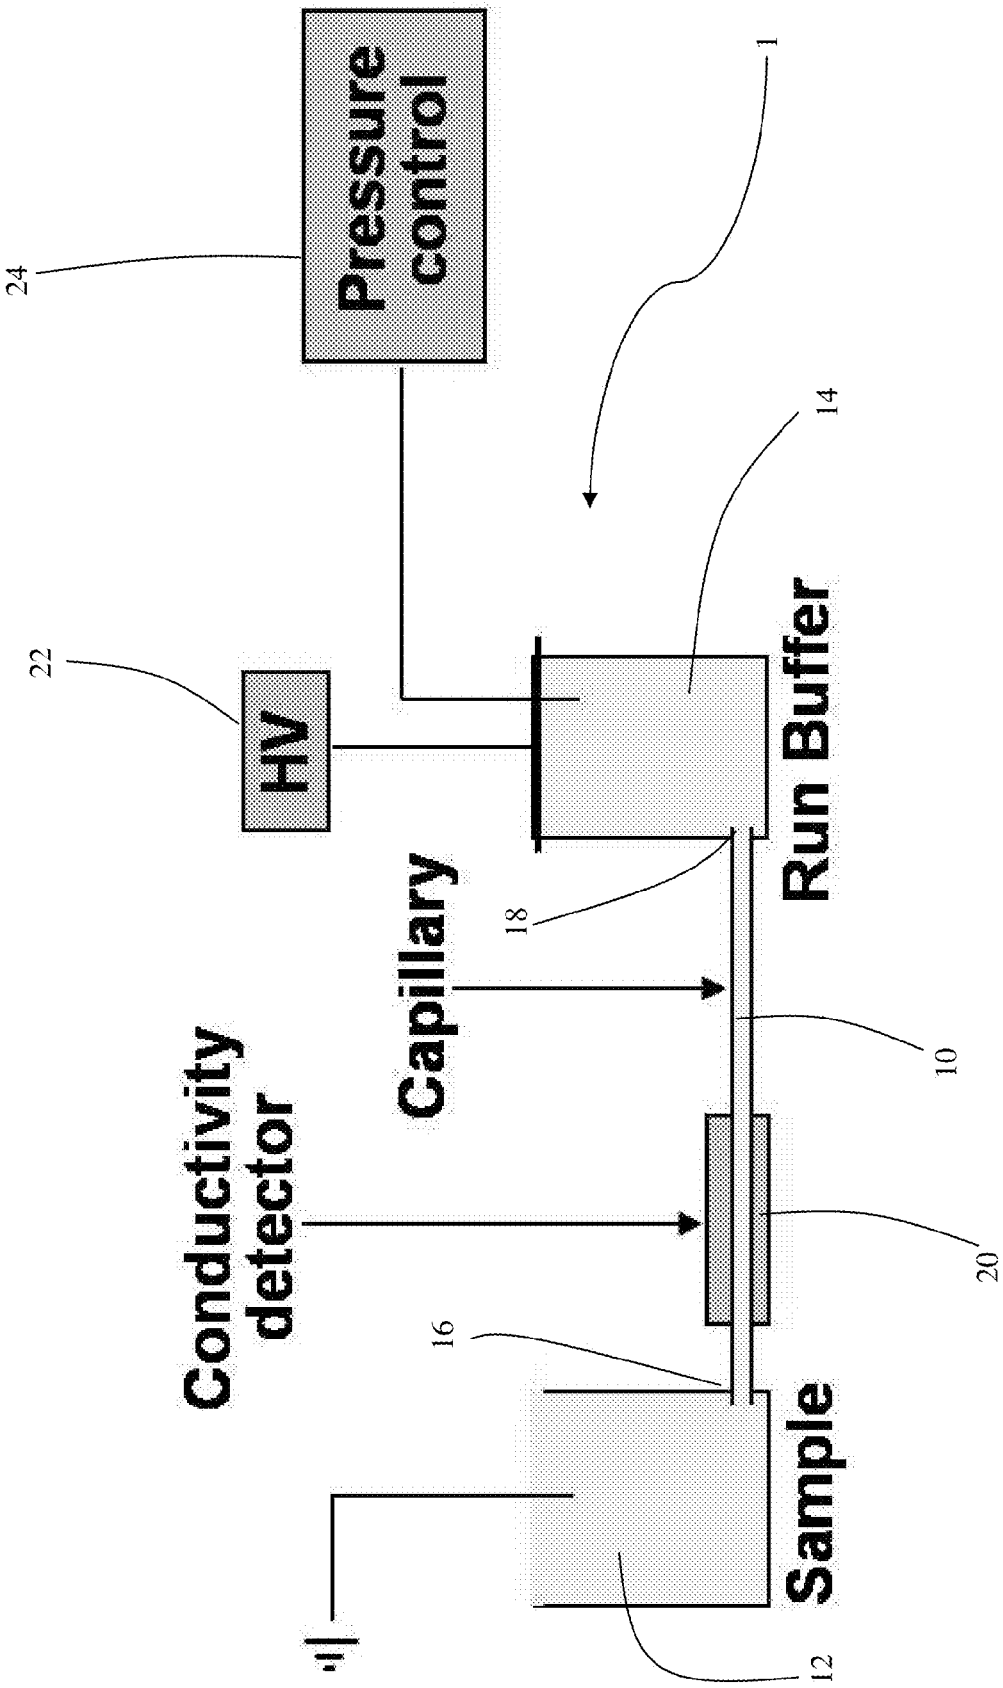
Pressure control
24
1
14
22
HV
Run Buffer
18
Capillary
10
Conductivity detector
20
16
Sample
12

FIG. 1