US008750541B1

(12) **United States Patent**
Dong et al.

(10) **Patent No.: US 8,750,541 B1**
(45) **Date of Patent: Jun. 10, 2014**

(54) **PARAMETRIC ARRAY FOR A HEAD-MOUNTABLE DEVICE**

(71) Applicant: **Google Inc.**, Mountain View, CA (US)

(72) Inventors: **Jianchun Dong**, Mountain View, CA (US); **Eliot Kim**, Mountain View, CA (US); **Mitchell J. Heinrich**, Mountain View, CA (US)

(73) Assignee: **Google Inc.**, Mountain View, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **13/665,469**

(22) Filed: **Oct. 31, 2012**

(51) **Int. Cl.**
H04R 25/00 (2006.01)

(52) **U.S. Cl.**
USPC **381/182**; 381/370; 381/374; 381/310

(58) **Field of Classification Search**
USPC 381/182–186, 310
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,532,292	B1 *	3/2003	Lygas	381/74
6,746,402	B2	6/2004	Ustuner	
7,130,430	B2	10/2006	Milsap	
7,146,011	B2	12/2006	Yang et al.	
7,190,378	B2	3/2007	Sauer et al.	
8,000,170	B2	8/2011	Kablotsky	
8,040,292	B2 *	10/2011	Ronzani et al.	345/8
2003/0215103	A1 *	11/2003	Norris et al.	381/77
2006/0132382	A1	6/2006	Jannard	
2008/0159571	A1 *	7/2008	Hooley	381/307
2008/0279410	A1 *	11/2008	Cheung et al.	381/381
2010/0074460	A1	3/2010	Marzetta	
2010/0149073	A1	6/2010	Chaum et al.	
2011/0245670	A1	10/2011	Tashiro et al.	
2012/0075168	A1	3/2012	Osterhout et al.	

FOREIGN PATENT DOCUMENTS

WO 2011045613 A1 4/2011

OTHER PUBLICATIONS

Bajura, Michael et al., "Merging Virtual Objects with the Real World: Seeing Ultrasound Imagery within the Patient," Computer Graphics, 26; Jul. 2, 1992.

* cited by examiner

Primary Examiner — Curtis Kuntz
Assistant Examiner — Ryan Robinson
(74) *Attorney, Agent, or Firm* — McDonnell Boehnen Hulbert & Berghoff LLP

(57) **ABSTRACT**

An apparatus includes a head-mountable support structure, a transducer array coupled to the support structure, and a processor configured to control the transducer array to radiate ultrasonic waves toward an ear of a user of the head-mountable support structure. The ultrasonic waves are audible.
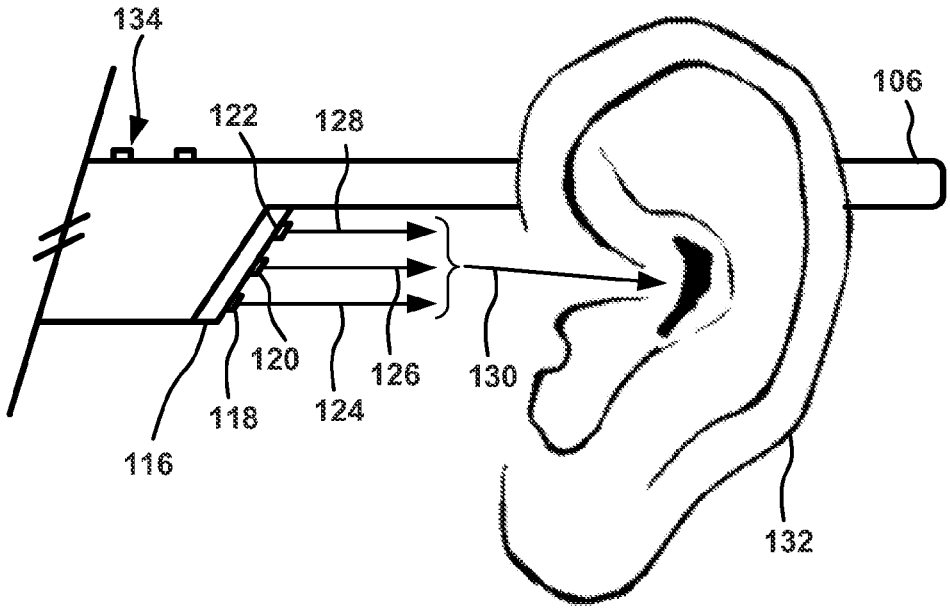
18 Claims, 5 Drawing Sheets